



HAL
open science

**Corrigendum: Measurement of thermodynamic
temperature between 5 K and 24.5 K with
Single-Pressure Refractive-Index Gas Thermometry
(2020 Metrologia 57 065006)**

Bo Gao, Haiyang Zhang, Dongxu Han, Changzhao Pan, Hui Chen, Yaonan Song, Wenjing Liu, Jiangfeng Hu, Xiangjie Kong, Fernando Sparasci, et al.

► **To cite this version:**

Bo Gao, Haiyang Zhang, Dongxu Han, Changzhao Pan, Hui Chen, et al.. Corrigendum: Measurement of thermodynamic temperature between 5 K and 24.5 K with Single-Pressure Refractive-Index Gas Thermometry (2020 Metrologia 57 065006). Metrologia, 2021, 58 (5), pp.059501. 10.1088/1681-7575/ac1e04 . hal-03959944

HAL Id: hal-03959944

<https://cnam.hal.science/hal-03959944>

Submitted on 10 Mar 2023

HAL is a multi-disciplinary open access archive for the deposit and dissemination of scientific research documents, whether they are published or not. The documents may come from teaching and research institutions in France or abroad, or from public or private research centers.

L'archive ouverte pluridisciplinaire **HAL**, est destinée au dépôt et à la diffusion de documents scientifiques de niveau recherche, publiés ou non, émanant des établissements d'enseignement et de recherche français ou étrangers, des laboratoires publics ou privés.



CORRIGENDUM • OPEN ACCESS

Corrigendum: Measurement of thermodynamic temperature between 5 K and 24.5 K with Single-Pressure Refractive-Index Gas Thermometry (2020 *Metrologia* [57 065006](#))

To cite this article: Bo Gao *et al* 2021 *Metrologia* **58** 059501

View the [article online](#) for updates and enhancements.

You may also like

- [Primary thermometry at 4 K, 14 K, and 25 K applying dielectric-constant gas thermometry](#)
Christof Gaiser and Bernd Fellmuth
- [Gas flow standards and their uncertainty](#)
John D Wright, Shin-Ichi Nakao, Aaron N Johnson *et al.*
- [Defining relative humidity in terms of water activity. III. Relations to dew-point and frost-point temperatures](#)
Rainer Feistel, Olaf Hellmuth and Jeremy Lovell-Smith

Corrigendum

Corrigendum: Measurement of thermodynamic temperature between 5 K and 24.5 K with Single-Pressure Refractive-Index Gas Thermometry (2020 *Metrologia* 57 065006)

Bo Gao^{1,2,*} , Haiyang Zhang^{1,2} , Dongxu Han^{1,3}, Changzhao Pan^{1,4} , Hui Chen², Yaonan Song^{1,2,5}, Wenjing Liu^{1,2,5}, Jiangfeng Hu^{1,2,5}, Xiangjie Kong^{1,2,5}, Fernando Sparasci^{1,4} , Mark Plimmer^{1,4} , Ercang Luo^{1,2,5,*} and Laurent Pitre^{1,4,*} 

¹ TIPC-LNE Joint Laboratory on Cryogenic Metrology Science and Technology, Technical Institute of Physics and Chemistry (TIPC), Chinese Academy of Sciences (CAS), Beijing 100190, People's Republic of China

² CAS Key Laboratory of Cryogenics, Technical Institute of Physics and Chemistry, Chinese Academy of Sciences, Beijing 100190, People's Republic of China

³ School of Mechanical Engineering, Beijing Institute of Petrochemical Technology, Beijing 102617, People's Republic of China

⁴ Laboratoire national de métrologie et d'essais-Conservatoire national des arts et métiers (LNE-Cnam), F93210, La Plaine-Saint Denis, France

⁵ University of Chinese Academy of Sciences, Beijing 100490, People's Republic of China

E-mail: bgao@mail.ipc.ac.cn, ecluo@mail.ipc.ac.cn and laurent.pitre@cnam.fr

Received 9 June 2021, revised 26 July 2021

Accepted for publication 16 August 2021

Published 14 September 2021



CrossMark

(Some figures may appear in colour only in the online journal)

We have corrected T and $T - T_{90}$ results in table 9 and figure 34 of the original paper (*Metrologia* 2020 57 065006) for the following reasons:

1. An incorrect value of the sensitivity of the standard platinum cobalt resistance thermometer (Chino RS144.08), used to transfer the reference thermodynamic temperature T_{ref} to the

single-pressure refractive-index gas thermometry (SPRIGT) system, was used. The manufacturer specification, used in the original paper gives $dR/dT = 0.1291 \Omega \text{ K}^{-1}$. Post-publication, we checked the value experimentally and found it be $0.1714 (4) \Omega \text{ K}^{-1}$.

2. The value of the reference thermodynamic temperature T^* used in an acoustic AGT paper [1] in which the same reference thermometer was employed, the difference being $42 \mu\text{K}$ at temperatures close to 24.6 K, namely 24.554 948(158) K to 24.554 990(160) K.

As shown in the corrected versions of table 9 and figure 34, the combined effect of the above terms is to lower the

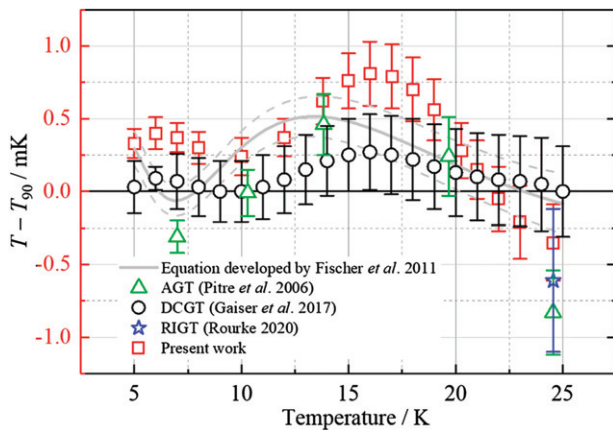
* Authors to whom any correspondence should be addressed.



Original content from this work may be used under the terms of the [Creative Commons Attribution 4.0 licence](https://creativecommons.org/licenses/by/4.0/). Any further distribution of this work must maintain attribution to the author(s) and the title of the work, journal citation and DOI.

Table 9. Corrected values of $T_{\text{SPRIGT}} - T_{90,\text{CAS}}$ in the present work. The first four columns of this table replace the data in table 9 of the original paper. The last two columns show the size of the downward temperature shift, which never exceeds 0.24 mK.

$T_{\text{SPRIGT}}^{\text{a}}$	$u(T_{\text{SPRIGT}})^{\text{a}}$	$T_{\text{SPRIGT}} - T_{90,\text{CAS}}^{\text{a}}$	$u(T_{\text{SPRIGT}} - T_{90,\text{CAS}})^{\text{a}}$	$\Delta T_{\text{SPRIGT}}^{\text{b}}$	$\frac{ \Delta T_{\text{SPRIGT}} }{u(T_{\text{SPRIGT}})}$
K	mK	mK	mK	mK	/
24.55535	0.16	-0.35	0.26	-0.24	1.50
23.00025	0.15	-0.21	0.25	-0.21	1.40
21.99973	0.13	-0.05	0.22	-0.19	1.46
20.99828	0.12	0.15	0.20	-0.18	1.50
20.26790	0.11	0.28	0.19	-0.16	1.45
18.99873	0.10	0.56	0.21	-0.14	1.40
17.99977	0.09	0.70	0.22	-0.13	1.44
17.03389	0.09	0.79	0.22	-0.11	1.22
16.00012	0.08	0.81	0.22	-0.10	1.25
15.00062	0.07	0.76	0.19	-0.08	1.14
13.80428	0.07	0.62	0.16	-0.07	1.00
12.00052	0.06	0.37	0.13	-0.06	1.00
10.00094	0.05	0.24	0.13	-0.04	0.80
8.00097	0.05	0.30	0.11	-0.03	0.60
7.00026	0.05	0.37	0.10	-0.02	0.40
6.00006	0.05	0.40	0.11	-0.02	0.40
5.00021	0.06	0.33	0.10	-0.02	0.33

^aCorrected values in this paper.^b $\Delta T_{\text{SPRIGT}} = T_{\text{SPRIGT}} - T_{\text{SPRIGT,old}}$, where $T_{\text{SPRIGT,old}}$ are taken from table 9 in the original paper.**Figure 34.** Weighted mean of $(T - T_{90})$ and comparison with the most recently available world average values (the grey lines) calculated using the equation developed by Fischer *et al* [4] and recent results obtained by AGT [53], DCGT [66] and RIGT [67] in the same temperature range. This figure replaces figure 34 of the original paper, the references numbers being the same.

determined thermodynamic temperature T_{SPRIGT} by at most 0.24 mK. This difference is due to the fact that the reference temperatures calibrated using in AGT in France and the setpoint of SPRIGT in China differed by 0.86 mK. Had

both experiments used an identical value of *resistance*, no correction would have been necessary.

Note: In the re-analysis of SPRIGT data, for completeness, the most recent and accurate value of the second dielectric virial coefficient B_ϵ [2] was used. The effect on the temperatures is less than 7 μK at temperatures close to 5 K and much smaller at other temperature.

ORCID iDs

Bo Gao <https://orcid.org/0000-0002-7277-5150>Haiyang Zhang <https://orcid.org/0000-0002-3303-8975>Changzhao Pan <https://orcid.org/0000-0002-1473-2582>Fernando Sparasci <https://orcid.org/0000-0002-9130-4338>Mark Plimmer <https://orcid.org/0000-0001-8727-2997>Laurent Pitre <https://orcid.org/0000-0001-9885-7544>

References

- [1] Pan C *et al* 2021 Acoustic measurement of the triple point of neon T_{Ne} and thermodynamic calibration of a transfer standard for accurate cryogenic thermometry *Metrologia* **58** 045006
- [2] Garberoglio G and Harvey A H 2020 Path-integral calculation of the second dielectric and refractivity virial coefficients of helium, neon, and argon *J. Res. Natl. Inst. Stan.* **125** 125022